

Medizinische Einweg OP – Maske Type IIR mit Spritzschutz, unsteril, EN 14683: 2019 + AC: 2019, CE



Merkmale der medizinischen Einweg-OP-Maske, Typ IIR – EN 14683: 2019 + AC: 2019

- Erfüllt die neueste Norm für **Typ IIR** Masken – **EN 14683: 2019 + AC: 2019**
- **ISO 9001 / 14001 / 45001** und **CE EC-REP**
- Bakterielle Filterleistung (**BFE**): **≥ 98 %**
- **EMPA Prüfbericht: Prüfbericht Nr. 5214025580-G**
- **Type IIR** Splash Resistance nach **ISO 22609: 2004**
- **Schützt Träger und Mitmenschen mittels hochwirksamen 3-Lagen-Vlies**
- **Hochqualitatives Vlies**, hergestellt im melt-blown Verfahren
- **Speziell spritzfeste Aussen-Beschichtung** zum Schutz vor Blut und anderen Körperflüssigkeiten mit **30g / m² beschichtetem Vlies**
- **CE / EC-REP**
- **Testreport von SGS**, ein weltweit führende Unternehmen in den Bereichen Prüfen, Testen, Verifizieren und Zertifizieren mit Sitz in Genf (www.sgs.ch)
- **Zusätzlich SGS SVHC-Test vorhanden** (Substances of Very High Concern) bieten Unternehmen, Verbrauchern und Endverbrauchern die Gewissheit, dass getestete Produkte und Materialien keine schädlichen Mengen an Chemikalien enthalten, die für die menschliche Gesundheit und die Umwelt gefährlich sind
- **Permanente, rollende Qualitätsüberwachung mittels Q-Tests vom Importeur bei SGS** durchgeführt
- 4-sprachige Verpackung und User-Manual
- **Amfori BSCI zertifizierter** von BVQ / Weltklasse-Tools zur Steuerung der sozialen und ökologischen Leistung der ganzen Lieferketten & Herstellung www.amfori.org

Technische Daten

- EN 14683: 2019 + AC: 2019 Type IIR Einweg-Schutzmasken mit Ohrengummis
- Type IIR: Spritzfeste Schicht zum Schutz vor Blut und anderen Körperflüssigkeiten
- nicht steril, für Einmalgebrauch
- Bakterielle Filterleistung (Bacteria Filter Efficiency - BFE): $\geq 98 \%$
- ISO 9001 / 14001 / 45001 und CE EC-REP
- Faltausführung mit elastischen Ohrschlingen
- Wirksamer 3-Lagen-Typ IIR Schutz aus hochqualitativem Vlies
 - 1. Lage: Auslaufsicherer Vliesstoff (hell-blau, 30g / m²)
 - 2. Lage: Hochdichtes schmelzgeblasenes Filtergewebe
 - 3. Lage: Vliesschicht für direkten Hautkontakt
- Integrierter biegbarer, versiegelter Nasenbügel
- Latex und glasfaserfrei
- Hoher Tragkomfort, kann auch von Brillenträgern getragen werden
- Die leichte Ohrbügelmaske lässt sich einfach aufsetzen und entfernen
- Sie ist bequem und es ist leicht zu atmen
- Maskengrösse: 17.5 x 9.5 cm
- Verpackungseinheit: 50er-Packung per Box / 2'500 Box per Karton / 40'000 Stk. per Palette, Verpackung mit EAN Bar Code, Qualitäts-Bestätigung mit Lot-Nr. in Box
- 2500 Stk. / Karton, Brutto-Gewicht 11.1kg, Grösse 55*41*39 cm
- Haltbarkeit 2 Jahre, Datum aufgedruckt auf jeder Box

Was	Details	Bemerkung
China Ministry of Commerce White List Producer	Ja	CE
CE Certificate	Lotus BV NL as EU Representative	EC REP
Test Report by	SGS & EMPA	Swiss certification institution
Applied standard	EN 14683:2019+AC2019	Type II R
Factory ISO Certificates	9001 / 14001 / 45001	
Product classification	Medical Use	
Sterile / Non Sterile	Non Sterile	
Packaging	50 pcs/ box 2500 pcs/ ctn 11.1 kg / ctn	

Technisches KNOW-HOW

Prüfung	Typ I	Typ I R	Typ II	Typ II R
Bakterielle Filterleistung	≥95 %	≥95 %	≥98 %	≥98 %
Druckdifferenz Pa	< 29,4	< 49,0	< 29,4	< 49,0
Druck des Spritzwiderstandes mm Hg	entfällt	≥120	entfällt	≥120
Widerstandsfähig gegen Flüssigkeitsspritzer		ja		ja

Typ II ist also besser als Typ I und R bedeutet höhere Beständigkeit gegen Flüssigkeiten und Aerosole.

Einweg Medical Type IIR mit Spritzschutz

Medizinische Gesichtsmasken des Typ IIR schützen den Träger und andere Personen. Sie reduzieren einen Kontakt des Trägers mit grossen, ausgeworfenen Teilchen einer erkrankten Person (z.B. Speichel, Schleim);

Sie schützt ausserdem den Träger vor Blut und / oder anderen Körperflüssigkeiten des Patienten oder aus dem Arbeitsumfeld.

Masken des Typs IIR – EN 14683: 2019 + AC: 2019 sind geeignet für Situationen, in denen die/der medizinische Mitarbeiter das Risiko eines Kontakts mit Blut und/oder anderen Körperflüssigkeiten des Patienten oder aus dem Arbeitsumfeld besteht oder für den privaten Gebrauch **zum Eigenschutz und Schutz der Mitmenschen.**

SGS -Test EN 14683: 2019 + AC: 2019 und ISO 22609:2004 (mit Spritzschutz)



中国认可
国际互认
检测
TESTING
CNAS L0599

Test Report SL52025233812101TX **Date:** April 17, 2020 **Page 1 of 3**
SHANDONG POP JEANS INTELLIGENT MANUFACTURING CO.,LTD
NO.188 GENGJIAO ROAD, HUANTAI, ZIBO,SHANDONG, CHINA

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)Disposable face mask

Composition : Inner and outer 100% spunbond nonwovens/middle layer Melt blown nonwovens

Style No. : SN20200003

Sample Color : (A)Light Blue

Manufacturer : SHANDONG POP JEANS INTELLIGENT MANUFACTURING CO.,LTD

Supplier : SHANDONG POP JEANS INTELLIGENT MANUFACTURING CO.,LTD

Exported to : European union

Proposed Care Instruction : -

Sample Receiving Date : Mar 31,2020

Testing Period : Mar 31,2020 - Apr 17,2020

Test Result(s) : For further details, please refer to the following page(s).

Test Performed : Selected test(s) as requested by applicant

Signed for and on behalf of
SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Sara Guo (Account Executive)



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/sgs/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/sgs/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction clauses defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-705)8337 9443, or email: CN_Doccheck@sgs.com

3rd Building, No.889, Yishan Road, Xuhai District Shanghai, China 200233 t (86-21) 61400666 f (86-21) 64968793 www.sgs.com
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61400666 f (86-21) 64968793 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Test Result

Medical Face Masks-Requirements and Test Methods
(EN 14683:2019)

Clause 5.2.2 Bacterial filtration efficiency (BFE)@**

	1#	2#	3#	4#	5#
(BFE), %	99.8	99.6	99.7	99.7	99.6

Remark: Performance Requirement: Type I>95%, Type II>98%, Type IIR >98%

** : The test was carried out by external laboratory assessed as competent

@ : These test methods are not in CNAS accredited scope

Clause 5.2.3 Breathability

(EN 14683 :2019 Annex C, Flow rate 8 l/min)

Sample: A

	1#	2#	3#	4#	5#
Differential pressure ΔP (Pa/cm ²)	37.9	34.4	33.5	32.0	26.8

Remark: Performance Requirement: Type I<40 Pa/cm², Type II<40 Pa/cm², Type IIR<60 Pa/cm²

Clause 5.2.4 Splash Resistance

(ISO 22609 :2004, Pressure 16.0 kPa)

Sample: A

Penetration on inside surface

1#	2#	3#	4#	5#	6#	7#	8#
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass
9#	10#	11#	12#	13#	14#	15#	16#
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass
17#	18#	19#	20#	21#	22#	23#	24#
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass
25#	26#	27#	28#	29#	30#	31#	32#
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass

Number of Pass: 32

Overall result: Acceptable

Remark:

- 1) Performance Requirement Type I: N/A, Type II: N/A, Type IIR:≥16.0kPa
- 2) Distance of the medical face mask target area surface to the tip of cannula is 300±10mm.
- 3) Condition and Test temperature (21±5)°C, relative humidity (85±10)%
- 4) An acceptable quality limit of 4.0% is met for a single sampling plan when 29 or more of the 32 tested specimens show pass results



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/term-and-conditions> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/term-and-conditions/term-e-document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction clauses defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (86-755)8397 1442, or email: CN.Doccheck@sgs.com
3rd Building No.889, Yixian Road, Xuhai District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64956793 www.sgs.com.cn
中国·上海·徐汇区宜山路889号5号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64956793 e sgs.china@sgs.com



中国认可
国际互认
检测
TESTING
CNAS L0599

Test Report

SL52025233812101TX

Date: April 17, 2020

Page 3 of 3

Clause 5.2.5 Microbial Cleanliness
(EN 14683: 2019 Annex D)

	1#	2#	3#	4#	5#
CFU/g	<1	<1	<1	<1	<1

Remark: Performance Requirement: Type I≤30 CFU/g, Type II≤30 CFU/g, Type IIR≤30 CFU/g

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/terms-and-conditions/terms-a-document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not constitute parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (86-755) 8307 5442, or email: CN_Speccheck@sgs.com

丁 Building No.888 Xiang-Yuan Road, Xuhui District, Shanghai, China 200233 | (86-21) 61402666 | (86-21) 64656763 | www.sgs.com
中国·上海·徐汇区宜山路888号3号楼 邮编: 200233 | (86-21) 61402666 | (86-21) 64656763 | sgs.china@sgs.com

Member of the SGS Group (SGS SA)

SGS SVHC-Test (Substances of Very High Concern) / Test bezüglich schädliche Mengen an Chemikalien



Test Report **SL22002253220301TX** **Date: May 20, 2020** **Page 1 of 16**
SHANDONG POP JEANS INTELLIGENT MANUFACTURING CO.,LTD
188 GENGJIAO ROAD, HUANTAI COUNTY, ZIBO CITY, SHANDONG PROVINCE

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A) single-use medical face mask(non-sterile) in blue

Sample Receiving Date : May 14, 2020

Testing Period : May 14, 2020 - May 20, 2020

Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Test Performed : Selected test(s) as requested by applicant

Summary :

According to the ruling of the Court of Justice of the European Union on the definition of an article under REACH, and the specified scope and evaluation screening, the test results of SVHC are $\leq 0.1\%$ (w/w) in the articles of the submitted sample. **PASS**

Signed for and on behalf of
SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.


York Yao (Account Executive)



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.
Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone (+86-755) 8387 1882, or email: CS.Docscheck@sgs.com

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.
188 GENGJIAO ROAD, HUANTAI COUNTY, ZIBO CITY, SHANDONG PROVINCE

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (+86-532) 6869 9666 f (+86-532) 83864258 www.sgsgroup.com.cn
中国·青岛·城阳区长春路143号通检中心 邮编: 266101 t (+86-532) 6869 9666 f (+86-532) 83864258 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)



Test Report

SL22002253220301TX

Date: May 20, 2020

Page 2 of 16

SVHC

Test Sample :

Sample Description :

Specimen No.	SGS Sample ID	Description
SN1	TAO20-018009.001	non metal group
SN2	TAO20-018009.002	metal group

SGS Sample ID	Photo No.	Material Description
001	P1	Blue fabric
001	P2	White fabric
001	P3	White fabric
001	P4	White fabric
001	P5	White plastic
002	P6	Silvery metal

Test Result

Test Result: (Substances in the Candidate List of SVHC)

Batch	Substance Name	CAS No.	001 Concentration (%)	RL (%)
-	All tested SVHC in candidate list	-	ND	-

Test Result: (Substances in the Consultation List of potential SVHC)

Batch	Substance Name	CAS No.	001 Concentration (%)	RL (%)
-	All tested SVHC in consultation list	-	ND	-

Test Result: (Substances in the Candidate List of SVHC)

Batch	Substance Name	CAS No.	002 Concentration (%)	RL (%)
-	All tested SVHC in candidate list	-	ND	-



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/Terms-and-Conditions/Terms-a-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

SGS-CTI (China) Technical Services Co., Ltd.
 检测认证中心
 Testing Laboratory

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6859 9688 f (86-532) 83684258 www.sgs.com.cn
 中国·青岛·莱山区株洲路143号检测中心 邮编: 266101 t (86-532) 6859 9688 f (86-532) 83684258 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Notes :

1. The table above only shows detected SVHC, and SVHC that below RL are not reported.
Please refer to Appendix for the full list of tested SVHC.
2. RL = Reporting Limit (Test data will be shown if it \geq RL. RL is not regulatory limit.)
ND = Not detected (lower than RL), ND is denoted on the SVHC substance.
3. Δ CAS No. of diastereoisomers identified (α -HBCDD, β -HBCDD, γ -HBCDD): 134237-50-6, 134237-51-7, 134237-52-8
 \star CAS No. of Hexahydromethylphthalic anhydride, Hexahydro-4-methylphthalic anhydride, Hexahydro-1-methylphthalic anhydride, Hexahydro-3-methylphthalic anhydride: 25550-51-0, 19438-60-9, 48122-14-1, 57110-29-9; EC No. of those: 247-094-1, 243-072-0, 256-356-4, 260-566-1.
4. * The test result is based on the calculation of selected element(s) and to the worst-case scenario.
 ** The test result is based on the calculation of selected marker(s) and to the worst-case scenario.
 For detail information, please refer to the SGS REACH website: <http://www.sgs.com/en/Consumer-Goods-Retail-Toys-and-Juvenile-Products/Toys/REACH/Management-of-SVHC.aspx>
 Calculated concentration of boric compounds are based on the total boron for liquid, powder and paste samples and water extractive boron for other samples by ICP-OES.
 RL = 0.01% is evaluated for element (i.e. cobalt, arsenic, lead, chromium (VI), aluminum, zirconium, boron, strontium, zinc, antimony, titanium, barium and cadmium respectively), except molybdenum RL=0.001%, boron RL=0.005% (only for Lead bis(tetrafluoroborate), chromium (VI) RL=0.005% (only for Pentazinc chromate octahydroxide).
5. \S The substance is proposed for the identification as SVHC only where it contains Michler's ketone (CAS Number: 90-94-8) or Michler's base (CAS Number: 101-61-1) \geq 0.1% (w/w).
6. Composite test has been performed in equal proportion for the components/material per client requested. And the result is calculated using the minimum sample weight.
7. In consideration of the analysis requirement and the limit of sample volume, the screening test for the article is based on components / material enough to test.
8. / = Substances in the Consultation List of SVHC.



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/terms-and-conditions/terms-and-conditions.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in the test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
 Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6899 9688 f (86-532) 83864258 www.sgs.com.cn
 中国·青岛·莱山区株洲路143号通检中心 邮编: 266101 t (86-532) 6899 9688 f (86-532) 83864258 e sgs.china@sgs.com

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
I	1	4,4'-Diaminodiphenylmethane(MDA)	101-77-9	0.100
I	2	5-tert-butyl-2,4,6-trinitro-m-xylene (musk xylene)	81-15-2	0.100
I	3	Alkanes, C10-13, chloro (Short Chain Chlorinated Paraffins)	85535-84-8	0.100
I	4	Anthracene	120-12-7	0.100
I	5	Benzyl butyl phthalate (BBP)	85-68-7	0.100
I	6	Bis (2-ethylhexyl)phthalate (DEHP)	117-81-7	0.100
I	7	Bis(tributyltin)oxide (TBTO)	56-35-9	0.100
I	8	Cobalt dichloride*	7646-79-9	0.010
I	9	Diarsenic pentaoxide*	1303-28-2	0.010
I	10	Diarsenic trioxide*	1327-53-3	0.010
I	11	Dibutyl phthalate (DBP)	84-74-2	0.100
I	12	Hexabromocyclododecane (HBCDD) and all major diastereoisomers identified (α -HBCDD, β -HBCDD, γ -HBCDD) Δ	25637-99-4, 3194-55-6	0.100
I	13	Lead hydrogen arsenate*	7784-40-9	0.010
I	14	Sodium dichromate*	7789-12-0, 10588-01-9	0.010
I	15	Triethyl arsenate*	15606-95-8	0.010
II	16	2,4-Dinitrotoluene	121-14-2	0.100
II	17	Acrylamide	79-06-1	0.100
II	18	Anthracene oil**	90640-80-5	0.100
II	19	Anthracene oil, anthracene paste**	90640-81-6	0.100
II	20	Anthracene oil, anthracene paste, anthracene fraction**	91995-15-2	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Services-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8337 1443, or email: CN.Questions@sgs.com
 SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 | (86-532) 8899 9688 | (86-532) 83884258 | www.sgs.com
 中国·青岛·莱山区株洲路143号检测中心 | 邮编: 266101 | (86-532) 8899 9688 | (86-532) 83884258 | sgs.china@sgs.com



Test Report

SL22002253220301TX

Date: May 20, 2020

Page 5 of 16

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
II	21	Anthracene oil, anthracene paste, distr. lights**	91995-17-4	0.100
II	22	Anthracene oil, anthracene-low**	90640-82-7	0.100
II	23	Diisobutyl phthalate	84-69-5	0.100
II	24	Lead chromate molybdate sulphate red (C.I. Pigment Red 104)*	12656-85-8	0.010
II	25	Lead chromate*	7758-97-6	0.010
II	26	Lead sulfochromate yellow (C.I. Pigment Yellow 34)*	1344-37-2	0.010
II	27	Pitch, coal tar, high temp.**	65996-93-2	0.100
II	28	Tris(2-chloroethyl)phosphate	115-96-8	0.100
III	29	Ammonium dichromate*	7789-09-5	0.010
III	30	Boric acid*	10043-35-3, 11113-50-1	0.010
III	31	Disodium tetraborate, anhydrous*	1303-96-4, 1330-43-4, 12179-04-3	0.010
III	32	Potassium chromate*	7789-00-6	0.010
III	33	Potassium dichromate*	7778-50-9	0.010
III	34	Sodium chromate*	7775-11-3	0.010
III	35	Tetraboron disodium heptaoxide, hydrate*	12267-73-1	0.010
III	36	Trichloroethylene	79-01-6	0.100
IV	37	2-Ethoxyethanol	110-80-5	0.100
IV	38	2-Methoxyethanol	109-86-4	0.100
IV	39	Chromic acid, Oligomers of chromic acid and dichromic acid, Dichromic acid*	7738-94-5 - 13530-68-2	0.010



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

SGS (China) Technical Services Co., Ltd.
Tianjin Laboratory

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6999 9668 f (86-532) 83884258 www.sgs.com.cn
中国·青岛·城阳区株洲路143号检测中心 邮编: 266101 t (86-532) 6999 9668 f (86-532) 83884258 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
IV	40	Chromium trioxide*	1333-82-0	0.010
IV	41	Cobalt(II) carbonate*	513-79-1	0.010
IV	42	Cobalt(II) diacetate*	71-48-7	0.010
IV	43	Cobalt(II) dinitrate*	10141-05-6	0.010
IV	44	Cobalt(II) sulphate*	10124-43-3	0.010
V	45	1,2,3-trichloropropane	96-18-4	0.100
V	46	1,2-Benzenedicarboxylic acid, di-C6-8-branched alkyl esters, C7-rich	71888-89-6	0.100
V	47	1,2-Benzenedicarboxylic acid, di-C7-11-branched and linear alkyl esters	68515-42-4	0.100
V	48	1-methyl-2-pyrrolidone	872-50-4	0.100
V	49	2-ethoxyethyl acetate	111-15-9	0.100
V	50	Hydrazine	7803-57-8, 302-01-2	0.100
V	51	Strontium chromate*	7789-06-2	0.010
VI	52	1,2-Dichloroethane	107-06-2	0.100
VI	53	2,2'-dichloro-4,4'-methylenedianiline	101-14-4	0.100
VI	54	2-Methoxyaniline; o-Anisidine	90-04-0	0.100
VI	55	4-(1,1,3,3-tetramethylbutyl)phenol	140-66-9	0.100
VI	56	Aluminosilicate Refractory Ceramic Fibres *	650-017-00-8 (Index no.)	0.010
VI	57	Arsenic acid*	7778-39-4	0.010
VI	58	Bis(2-methoxyethyl) ether	111-96-6	0.100
VI	59	Bis(2-methoxyethyl) phthalate	117-82-8	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitations of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8107 1643, or email: CN-Doccheck@sgs.com
 SGS Center, No. 143, Zhuzhou Road, Luoshan District, Qingdao, China 266101 t (86-532) 6999 9666 f (86-532) 63664258 www.sgs.com.cn
 中国·青岛·城阳区株洲路143号通检中心 邮编: 266101 t (86-532) 6999 9666 f (86-532) 63664258 e sgs.china@sgs.com

Appendix
Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
VI	60	Calcium arsenate*	7778-44-1	0.010
VI	61	Dichromium tris(chromate) *	24613-89-6	0.010
VI	62	Formaldehyde, oligomeric reaction products with aniline	25214-70-4	0.100
VI	63	Lead diazide, Lead azide*	13424-46-9	0.010
VI	64	Lead dipicrate*	6477-64-1	0.010
VI	65	Lead styphnate*	15245-44-0	0.010
VI	66	N,N-dimethylacetamide	127-19-5	0.100
VI	67	Pentazinc chromate octahydroxide*	49663-84-5	0.010
VI	68	Phenolphthalein	77-09-8	0.100
VI	69	Potassium hydroxyoctaoxidizincatedichromate*	11103-86-9	0.010
VI	70	Trilead diarsenate*	3687-31-8	0.010
VI	71	Zirconia Aluminosilicate Refractory Ceramic Fibres*	650-017-00-8 (Index no.)	0.010
VII	72	[4-[[4-anilino-1-naphthyl]]4-(dimethylamino)phenyl]methylene]cyclohexa-2,5-dien-1-ylidene] dimethylammonium chloride (C.I. Basic Blue 26)§	2580-56-5	0.100
VII	73	[4-[4,4'-bis(dimethylamino)benzhydrylidene]cyclohexa-2,5-dien-1-ylidene]dimethylammonium chloride (C.I. Basic Violet 3)§	548-62-9	0.100
VII	74	1,2-bis(2-methoxyethoxy)ethane (TEGDME; triglyme)	112-49-2	0.100
VII	75	1,2-dimethoxyethane; ethylene glycol dimethyl ether (EGDME)	110-71-4	0.100
VII	76	4,4'-bis(dimethylamino) benzophenone (Michler's Ketone)	90-94-8	0.100
VII	77	4,4'-bis(dimethylamino)-4''-(methylamino)trityl alcohol§	561-41-1	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/Terms-and-Conditions/Terms-Electronic-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-756) 8367 1443, or email: CN.Doccheck@sgs.com
 SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 8999 9668 f (86-532) 83884258 www.sgs.com.cn
 中国·青岛·莱山区株洲路143号检测中心 邮编: 266101 t (86-532) 8999 9668 f (86-532) 83884258 e sgs.china@sgs.com

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
VII	78	Diboron trioxide*	1303-86-2	0.010
VII	79	Formamide	75-12-7	0.100
VII	80	Lead(II) bis(methanesulfonate)*	17570-76-2	0.010
VII	81	N,N,N',N'-tetramethyl-4,4'-methylenedianiline (Michler's base)	101-61-1	0.100
VII	82	TGIC (1,3,5-tris(oxiranylmethyl)-1,3,5-triazine-2,4,6-(1H,3H,5H)-trione)	2451-62-9	0.100
VII	83	α,α-Bis[4-(dimethylamino)phenyl]-4 (phenylamino)naphthalene-1-methanol (C.I. Solvent Blue 4) §	6786-83-0	0.100
VII	84	β-TGIC (1,3,5-tris[(2S and 2R)-2,3-epoxypropyl]-1,3,5-triazine-2,4,6-(1H,3H,5H)-trione)	59653-74-6	0.100
VIII	85	[Phthalato(2-)]dioxotrilead*	69011-06-9	0.010
VIII	86	1,2-Benzenedicarboxylic acid, dipentylester, branched and linear	84777-06-0	0.100
VIII	87	1,2-Diethoxyethane	629-14-1	0.100
VIII	88	1-Bromopropane	106-94-5	0.100
VIII	89	3-Ethyl-2-methyl-2-(3-methylbutyl)-1,3-oxazolidine	143860-04-2	0.100
VIII	90	4-(1,1,3,3-tetramethylbutyl)phenol, ethoxylated	-	0.100
VIII	91	4,4'-Methylenedi-o-toluidine	838-88-0	0.100
VIII	92	4,4'-Oxydianiline and its salts	101-80-4	0.100
VIII	93	4-Aminoazobenzene	60-09-3	0.100
VIII	94	4-Methyl-m-phenylenediamine	95-80-7	0.100
VIII	95	4-Nonylphenol, branched and linear	-	0.100
VIII	96	6-Methoxy-m-toluidine	120-71-8	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone (+86-755) 8387 1663, or email: CN.Checback@sgs.com

SGS-CTI (Shanghai) Technical Service Co., Ltd.
检测认证

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (+86-532) 6889 9666 f (+86-532) 83864258 www.sgs.com.cn
中国·青岛·莱山区株洲路143号检测中心 邮编: 266101 t (+86-532) 6889 9666 f (+86-532) 83864258 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
VIII	97	Acetic acid, lead salt, basic*	51404-69-4	0.010
VIII	98	Biphenyl-4-ylamine	92-67-1	0.100
VIII	99	Bis(pentabromophenyl) ether (DecaBDE)	1163-19-5	0.100
VIII	100	Cyclohexane-1,2-dicarboxylic anhydride, cis-cyclohexane-1,2-dicarboxylic anhydride, trans-cyclohexane-1,2-dicarboxylic anhydride	85-42-7, 13149-00-3, 14166-21-3	0.100
VIII	101	Diazene-1,2-dicarboxamide (C,C'-azodi(formamide))	123-77-3	0.100
VIII	102	Dibutyltin dichloride (DBTC)	683-18-1	0.100
VIII	103	Diethyl sulphate	64-67-5	0.100
VIII	104	Diisopentylphthalate	605-50-5	0.100
VIII	105	Dimethyl sulphate	77-78-1	0.100
VIII	106	Dinoseb	88-85-7	0.100
VIII	107	Dioxobis(stearato)trilead*	12578-12-0	0.010
VIII	108	Fatty acids, C16-18, lead salts*	91031-62-8	0.010
VIII	109	Furan	110-00-9	0.100
VIII	110	Henicosfluoroundecanoic acid	2058-94-8	0.100
VIII	111	Heptacosfluorotetradecanoic acid	376-06-7	0.100
VIII	112	Hexahydromethylphthalic anhydride, Hexahydro-4-methylphthalic anhydride, Hexahydro-1-methylphthalic anhydride, Hexahydro-3-methylphthalic anhydride	☆	0.100
VIII	113	Lead bis(tetrafluoroborate)*	13814-96-5	0.010
VIII	114	Lead cyanamidate*	20837-86-9	0.010
VIII	115	Lead dinitrate*	10099-74-8	0.010



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1663, or email: CN.Doccheck@sgs.com

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6899 9688 f (86-532) 63884258 www.sgs.com.cn
 中国·青岛·城阳区株洲路143号检测中心 邮编: 266101 t (86-532) 6899 9688 f (86-532) 63884258 e sgs.china@sgs.com

Appendix
Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
VIII	116	Lead monoxide*	1317-36-8	0.010
VIII	117	Lead oxide sulfate*	12036-76-9	0.010
VIII	118	Lead tetroxide (orange lead)*	1314-41-6	0.010
VIII	119	Lead titanium trioxide*	12060-00-3	0.010
VIII	120	Lead titanium zirconium oxide*	12626-81-2	0.010
VIII	121	Methoxyacetic acid	625-45-6	0.100
VIII	122	Methyloxirane (Propylene oxide)	75-56-9	0.100
VIII	123	N,N-dimethylformamide	68-12-2	0.100
VIII	124	N-Methylacetamide	79-16-3	0.100
VIII	125	N-Pentyl-isopentylphthalate	776297-69-9	0.100
VIII	126	o-Aminoazotoluene	97-56-3	0.100
VIII	127	o-Toluidine	95-53-4	0.100
VIII	128	Pentacosfluorotridecanoic acid	72629-94-8	0.100
VIII	129	Pentalead tetraoxide sulphate*	12065-90-6	0.010
VIII	130	Pyrochlore, antimony lead yellow*	8012-00-8	0.010
VIII	131	Silicic acid, barium salt, lead-doped*	68784-75-8	0.010
VIII	132	Silicic acid, lead salt*	11120-22-2	0.010
VIII	133	Sulfurous acid, lead salt, dibasic*	62229-08-7	0.010
VIII	134	Tetraethyllead*	78-00-2	0.010
VIII	135	Tetralead trioxide sulphate*	12202-17-4	0.010
VIII	136	Tricosfluorododecanoic acid	307-55-1	0.100



SGS-CTI (Shanghai) Technical Service Co., Ltd.
Yantai Laboratory

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8387 1443, or email: Ch.Disc@back@sgs.com

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6889 9888 f (86-532) 63884258 www.sgsgroup.com.cn
中国·青岛·城阳区株洲路143号通检中心 邮编: 266101 t (86-532) 6889 9888 f (86-532) 63884258 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Appendix
Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
VIII	137	Trilead bis(carbonate)dihydroxide (basic lead carbonate)*	1319-46-6	0.010
VIII	138	Trilead dioxide phosphonate*	12141-20-7	0.010
IX	139	4-Nonylphenol, branched and linear, ethoxylated	-	0.100
IX	140	Ammonium pentadecafluorooctanoate (APFO)**	3825-26-1	0.100
IX	141	Cadmium oxide*	1306-19-0	0.010
IX	142	Cadmium*	7440-43-9	0.010
IX	143	Dipentyl phthalate (DPP)	131-18-0	0.100
IX	144	Pentadecafluorooctanoic acid (PFOA)	335-67-1	0.100
X	145	Cadmium sulphide*	1306-23-6	0.010
X	146	Dihexyl phthalate	84-75-3	0.100
X	147	Disodium 3,3'- [[1,1'-biphenyl]-4,4'-diylbis(azo)]bis(4-aminonaphthalene-1-sulphonate) (C.I. Direct Red 28)	573-58-0	0.100
X	148	Disodium 4-amino-3-[[4'-[(2,4-diaminophenyl)azo] [1,1'-biphenyl]-4-yl]azo]-5-hydroxy-6- (phenylazo)naphthalene-2,7-disulphonate (C.I. Direct Black 38)	1937-37-7	0.100
X	149	Imidazolidine-2-thione; 2-imidazoline-2-thiol	96-45-7	0.100
X	150	Lead di(acetate)*	301-04-2	0.010
X	151	Trixylyl phosphate	25155-23-1	0.100
XI	152	1,2-Benzenedicarboxylic acid, dihexyl ester, branched and linear	68515-50-4	0.100
XI	153	Cadmium chloride*	10108-64-2	0.010
XI	154	Sodium perborate; perboric acid, sodium salt*	-	0.010



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/terms-and-conditions/terms-and-conditions.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's Instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_Discover@sgs.com
 SGS Center, No. 143, Zhuzhou Road, Laxian District, Qingdao, China 266101 t (86-532) 6899 9688 f (86-532) 83684258 www.sgs.com.cn
 中国·青岛·城阳区株洲路143号检测中心 邮编: 266101 t (86-532) 6899 9688 f (86-532) 83684258 e sgs.china@sgs.com

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
XI	155	Sodium peroxometaborate*	7632-04-4	0.010
XII	156	2-(2H-benzotriazol-2-yl)-4,6-ditertpentylphenol (UV-328)	25973-55-1	0.100
XII	157	2-benzotriazol-2-yl-4,6-di-tert-butylphenol (UV-320)	3846-71-7	0.100
XII	158	2-ethylhexyl 10-ethyl-4,4-dioctyl-7-oxo-8-oxa-3,5-dithia-4-stannatetradecanoate (DOTE)	15571-58-1	0.100
XII	159	Cadmium fluoride*	7790-79-6	0.010
XII	160	Cadmium sulphate*	10124-36-4, 31119-53-6	0.010
XII	161	Reaction mass of 2-ethylhexyl 10-ethyl-4,4-dioctyl-7-oxo-8-oxa-3,5-dithia-4-stannatetradecanoate & 2-ethylhexyl 10-ethyl-4-[[2- [[2-ethylhexyl)oxy]-2-oxoethyl]thio]-4-octyl-7-oxo-8-oxa-3,5-dithia-4-stannatetradecanoate (reaction mass of DOTE & MOTE)	-	0.100
XIII	162	1,2-benzenedicarboxylic acid, di-C6-10-alkyl esters; 1,2-benzenedicarboxylic acid, mixed decyl and hexyl and octyl diesters with ≥ 0.3% of dihexyl phthalate	68515-51-5, 68648-93-1	0.100
XIII	163	5-sec-butyl-2- (2,4-dimethylcyclohex-3-en-1-yl)-5-methyl-1,3-dioxane [1], 5-sec-butyl-2- (4,6-dimethylcyclohex-3-en-1-yl)-5-methyl-1,3-dioxane [2] [covering any of the individual isomers of [1] and [2] or any combination thereof]	-	0.100
XIV	164	1,3-propanesultone	1120-71-4	0.100
XIV	165	2,4-di-tert-butyl-6-(5-chlorobenzotriazol-2-yl)phenol (UV-327)	3864-99-1	0.100
XIV	166	2-(2H-benzotriazol-2-yl)-4-(tert-butyl)-6-(sec-butyl)phenol (UV-350)	36437-37-3	0.100
XIV	167	Nitrobenzene	98-95-3	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8367 1683, or email: CN.Doccheck@sgs.com

SGS-CTI (Shanghai) Technical Services Co., Ltd.
Suzhou Laboratory

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6959 9668 f (86-532) 63864258 www.sgs.com.cn
中国·青岛·城阳区株洲路143号检测中心 邮编: 266101 t (86-532) 6959 9668 f (86-532) 63864258 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
XIV	168	Perfluorononan-1-oic-acid and its sodium and ammonium salts	375-95-1, 21049-39-8, 4149-60-4	0.100
XV	169	Benzo[def]chrysene (Benzo[a]pyrene)	50-32-8	0.100
XVI	170	4,4'-isopropylidenediphenol (bisphenol A)	80-05-7	0.100
XVI	171	4-Heptylphenol, branched and linear	-	0.100
XVI	172	Nonadecafluorodecanoic acid (PFDA) and its sodium and ammonium salts	3108-42-7, 335-76-2, 3830-45-3	0.100
XVI	173	p-(1,1-dimethylpropyl)phenol	80-46-6	0.100
XVII	174	Perfluorohexane-1-sulphonic acid and its salts	-	0.100
XVIII	175	1,6,7,8,9,14,15,16,17,17,18,18-Dodecachloropentacyclo[12.2.1.1.6,9.0.2,13.0.5,10]octadeca-7,15-diene ("Dechlorane Plus™") [covering any of its individual anti- and syn-isomers or any combination thereof]	-	0.100
XVIII	176	Benzo[a]anthracene	56-55-3, 1718-53-2	0.100
XVIII	177	Cadmium nitrate*	10022-68-1, 10325-94-7	0.010
XVIII	178	Cadmium carbonate*	513-78-0	0.010
XVIII	179	Cadmium hydroxide*	21041-95-2	0.010
XVIII	180	Chrysene	218-01-9, 1719-03-5	0.100
XVIII	181	Reaction products of 1,3,4-thiadiazolidine-2,5-dithione, formaldehyde and 4-heptylphenol, branched and linear (RP-HP) [with ≥0.1% w/w 4-heptylphenol, branched and linear]	-	0.100
XIX	182	Benzene-1,2,4-tricarboxylic acid 1,2-anhydride (trimellitic anhydride) (TMA)	552-30-7	0.100
XIX	183	Benzo[ghi]perylene	191-24-2	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/terms-and-conditions/terms-a-document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8387 1443, or email: CN.Doccheck@sgs.com

SGS (China) Technical Services (Shanghai) Co., Ltd.
Testing Laboratory

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 | (86-532) 6889 9688 | (86-532) 83864258 | www.sgs.com.cn
中国·青岛·棘洪滩路143号检测中心 | 邮编: 266101 | (86-532) 6889 9688 | (86-532) 83864258 | e sgs.china@sgs.com

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
XIX	184	Decamethylcyclotrasiloxane (D5)	541-02-6	0.100
XIX	185	Dicyclohexyl phthalate (DCHP)	84-61-7	0.100
XIX	186	Disodium octaborate*	12008-41-2	0.010
XIX	187	Dodecamethylcyclotrasiloxane (D6)	540-97-6	0.100
XIX	188	Ethylenediamine(EDA)	107-15-3	0.100
XIX	189	Lead*	7439-92-1	0.010
XIX	190	Octamethylcyclotetrasiloxane (D4)	556-67-2	0.100
XIX	191	Terphenyl, hydrogenated	61788-32-7	0.100
XX	192	1,7,7-trimethyl-3-(phenylmethylene)bicyclo[2.2.1]heptan-2-one (3-benzylidene camphor)	15087-24-8	0.100
XX	193	2,2-bis(4'-hydroxyphenyl)-4-methylpentane	6807-17-6	0.100
XX	194	Benzo[k]fluoranthene	207-08-9	0.100
XX	195	Fluoranthene	206-44-0, 93951-69-0	0.100
XX	196	Phenanthrene	85-01-8	0.100
XX	197	Pyrene	129-00-0, 1718-52-1	0.100
XXI	198	2,3,3,3-tetrafluoro-2-(heptafluoropropoxy)propionic acid, its salts and its acyl halides (covering any of their individual isomers and combinations thereof)	-	0.100
XXI	199	2-methoxyethyl acetate	110-49-6	0.100
XXI	200	4-tert-butylphenol (PTBP)	98-54-4	0.100
XXI	201	Tris(4-nonylphenyl, branched and linear) phosphite (TNPP) with ≥ 0.1% w/w of 4-nonylphenol, branched and linear (4-NP)	-	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/Terms-and-Conditions/Terms-Electronic.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1843, or email: CN.Doccheck@sgs.com

SGS-CTI (Shanghai) Technical Service Co., Ltd. | SGS Center, No. 143, Zhuzhou Road, Lixian District, Qingdao, China 266101 | (86-532) 6899 9688 | (86-532) 63884258 | www.sgs.com.cn
 中国·青岛·城阳区株洲路143号通检中心 | 邮编: 266101 | (86-532) 6899 9688 | (86-532) 63884258 | sgs.china@sgs.com

Appendix

Full list of tested SVHC:

Batch	No.	Substance Name	CAS No.	RL (%)
XXII	202	2-benzyl-2-dimethylamino-4'-morpholinobutyrophenone	119313-12-1	0.100
XXII	203	2-methyl-1-(4-methylthiophenyl)-2-morpholinopropan-1-one	71868-10-5	0.100
XXII	204	Diisohexyl phthalate	71850-09-4	0.100
XXII	205	Perfluorobutane sulfonic acid (PFBS) and its salts	-	0.100
/	206	1-vinylimidazole	1072-63-5	0.100
/	207	2-methylimidazole	693-98-1	0.100
/	208	Butyl 4-hydroxybenzoate	94-26-8	0.100
/	209	Dibutylbis(pentane-2,4-dionato-O,O')tin	22673-19-4	0.100
/	210	Resorcinol	108-46-3	0.100



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.cn/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.cn/Terms-and-Conditions/Terms-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8387 1443, or email: CN-Dispatch@sgs.com

SGS Center, No. 143, Zhuzhou Road, Laxian District, Qingdao, China 266101 | (86-532) 6959 9668 | (86-532) 83884258 | www.sgs.com.cn
 中国·青岛·城阳区株洲路143号检测中心 | 邮编: 266101 | (86-532) 6959 9668 | (86-532) 83884258 | sgs.china@sgs.com

SGS rollende Stichproben-Prüfungen der Lieferungen durch den Importeur



中国认可
国际互认
检测
TESTING
CNAS L0599

Test Report

SL52035285528301TX

Date: August 19, 2020

Page 1 of 3

SHANDONG POP JEANS INTELLIGENT MANUFACTURING CO.,LTD
NO. 188, GENGJIAO ROAD, HUANTAI, ZIBO, SHANDONG, CHINA

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)SINGLE-USE MEDICAL FACE MASK

Brand : ASPOP

Composition : (A)Polypropylene

Sample Color : (A)Blue

Style No. : SN2020000301

Order No. : ILB-SDP-ANT-004 (batch code 2020080110)

Manufacturer : SHANDONG POP JEANS INTELLIGENT MANUFACTURING CO.,LTD

Agent : ILB

Country of Destination : EUR

Test Performed : Selected test(s) as requested by applicant

Sample Receiving Date : Aug 11, 2020

Testing Period : Aug 11, 2020 - Aug 19, 2020

Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Signed for and on behalf of
SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Sara Guo (Account Executive)



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/terms-and-conditions/terms-e-document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not accrete parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Shanghai@sgs.com

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd
Testing Center

J Building, No. 888, Yixian Road, Xuhui District, Shanghai, China 200233 t (86-21) 61400666 f (86-21) 64556763 www.sgsgroup.com.cn
中国·上海·徐汇区宜山路888号3号楼 邮编: 200233 t (86-21) 61400666 f (86-21) 64556763 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Test Result

EN 14683:2019+AC:2019 Medical Face Masks-Requirements and Test Methods

Clause 5.2 Performance Requirement

Clause 5.2.4 Splash Resistance

(ISO 22609 :2004)

Sample: A

Test Blood Pressure : 16.0kPa

Pre-Conditioning : Minimum of 4 hours at 21±5°C and 85±5% R.H.

Distance of the mask to the tip of cannula : 300±10mm

Test Specimen#	Penetration on inside surface	Conclusion	Test Specimen#	Penetration on inside surface	Conclusion
1	None Seen	Pass	17	None Seen	Pass
2	None Seen	Pass	18	None Seen	Pass
3	None Seen	Pass	19	None Seen	Pass
4	None Seen	Pass	20	None Seen	Pass
5	None Seen	Pass	21	None Seen	Pass
6	None Seen	Pass	22	None Seen	Pass
7	None Seen	Pass	23	None Seen	Pass
8	None Seen	Pass	24	None Seen	Pass
9	None Seen	Pass	25	None Seen	Pass
10	None Seen	Pass	26	None Seen	Pass
11	None Seen	Pass	27	None Seen	Pass
12	None Seen	Pass	28	None Seen	Pass
13	None Seen	Pass	29	None Seen	Pass
14	None Seen	Pass	30	None Seen	Pass
15	None Seen	Pass	31	None Seen	Pass
16	None Seen	Pass	32	None Seen	Pass
Number of Pass:			32		
Overall result:			Acceptable		

Remark:

- 1) Performance Requirement Type I: N/A, Type II: N/A, Type IIR: ≥16.0kPa
- 2) Test was conducted within 60s after removal from conditioning chamber.
- 3) An acceptable quality limit of 4.0% is met for a single sampling plan when 29 or more of the 32 tested specimens show pass results.



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/terms-and-conditions/terms-e-document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction clauses defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8387 1443, or email: CN_Devcheck@sgs.com
 J'Building, No.888, Yotian Road, Xuhui District Shanghai, China 200233 t (86-21) 61400666 f (86-21) 64558753 www.sgs.com.cn
 中国·上海·徐汇区宜山路888号9号楼 邮编: 200233 t (86-21) 61400666 f (86-21) 64558753 e sgs.china@sgs.com



中国认可
国际互认
检测
TESTING
CNAS L0599


Test Report

SL52035285528301TX

Date: August 19, 2020

Page 3 of 3

Sample Photo

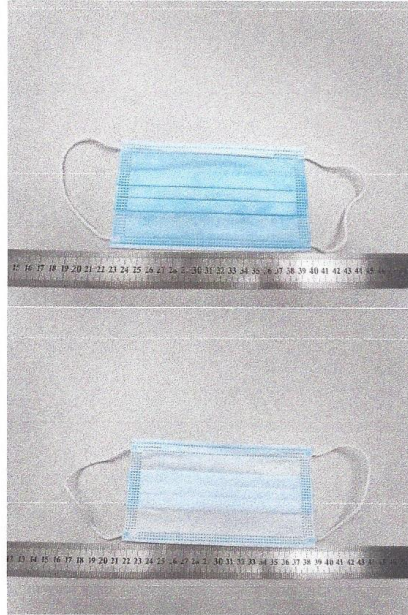

The statement of conformity in this test report is only based on measured values by the laboratory and does not take their uncertainties into consideration.

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/terms-and-conditions/terms-g-document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

SGS-OS (Shanghai) Technical Services (Shanghai) Co., Ltd.
Testing Center: No. 889, Yehan Road, Xuhui District, Shanghai, China

200233 t (86-21) 61402666 f (86-21) 64958763 www.sgs.com.cn
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Hersteller ist nach amfori - BSCI Verhaltenscodex Zertifikat von Bureau Veritas zertifiziert (<https://ch.amfori.org/de>)

Producer : Shandong Aspop Costumes Group Inc.

DBID : 351951 and Audit Id : 156209
Audit Type : Follow-up Audit

Audit Date : 05/07/2019



Auditee :	Shandong Aspop Costumes Group Inc.
Audit Date From :	05/07/2019
Audit Date To :	05/07/2019
Expiry Date of the Audit :	Please refer to the producer profile in the amfori BSCI platform
Auditing Company :	BureauVeritas
Auditor's Name(s) :	Michael Ma(Lead), Jordan LI
Auditing Branch (If applicable) :	



This is an extract of the on line Audit Report. The complete report is available in the amfori BSCI Platform.
Access www.bsclplatform.org, for entitled users only.

All rights reserved. No part of this publication may be reproduced, translated, stored in a retrieval system, or transmitted, in any form or by any means electronic, mechanical, photocopying, recording or otherwise, be lent, re-sold, hired out or otherwise circulated without the amfori consent.

This is an extract of the amfori BSCI Audit Report, which is available in the amfori BSCI Platform. © amfori, 2018 - The English version is the legally binding One.



GUOJIAN CERTIFICATION CO., LTD.

QUALITY MANAGEMENT SYSTEM CERTIFICATION

No: 174Q200145R0M

This is to certify that the quality system of

**SHANDONG POP JEANS
INTELLIGENT MANUFACTURING CO.,LTD.**

NO.188,GENGJIAO ROAD,TANGSHAN TOWN,HUANTAI COUNTY,ZIBO CITY,SHANDONG PROVINCE

Unified Social Credit Code: 913703213342969729

Quality Management System

Has been awarded this certificate for compliance with the standard

GB/T 19001-2016/ISO 9001:2015

This Quality Management System is valid for the

**RESEARCH & DEVELOPMENT, PRODUCTION AND SALE OF
PERSONALIZED CUSTOMIZED CLOTHING; PRODUCTION AND SALE OF ASPOP
BRAND CLOTHING; PRODUCTION AND SALE OF NON-MEDICAL DISPOSABLE ISOLATION GOWN**

(If the above scope involves pre-approval of administration permission and compulsory certification, this certificate only covers products/services in the approved / certified scope.)

Date of issue: 2020-06-22

Term of validity of this certificate: From 2020-06-22 to 2023-06-21

This certificate remains valid only if the certified organization accepts and passes regular surveillance audits.



Scan the QR code to check the validity of this certificate



Representative of The Certification Body



中国认可
国际互认
管理体系
MANAGEMENT SYSTEM
CNAS C169-M

The validity of this certificate could be confirmed via official Website of CNCA (www.cnca.gov.cn) Or the Website of Certification Body (www.cqsg.com) or contact 8611-6218299 ROOM 801, JUCHENGSHANDE BUILDING, NO.212 CENTRAL SHENGENG ROAD, JINAN CITY, SHANDONG PROVINCE, CHINA (250002) SHANDONG GUOJIAN CERTIFICATION CO., LTD.



GUOJIAN CERTIFICATION CO., LTD.

ENVIRONMENTAL MANAGEMENT SYSTEM CERTIFICATE

No: 174E200089R0M

This is to certify that the Environmental Management system of

**SHANDONG POP JEANS
INTELLIGENT MANUFACTURING CO.,LTD.**

NO.188,GENGJIAO ROAD,TANGSHAN TOWN,HUANTAI COUNTY,ZIBO CITY,SHANDONG PROVINCE

Unified Social Credit Code: 913703213342969729

Environmental Management System

Has been awarded this certificate for compliance with the standard

GB/T 24001-2016/ISO 14001:2015

This Environmental Management System is valid for the

**THE RELATIVE MANAGEMENT ACTIVITIES OF RESEARCH & DEVELOPMENT, PRODUCTION
AND SALE OF PERSONALIZED CUSTOMIZED CLOTHING; PRODUCTION AND SALE OF ASPOP
BRAND CLOTHING; PRODUCTION AND SALE OF NON-MEDICAL DISPOSABLE ISOLATION GOWN**

(If the above scope involves pre-approval of administration permission and compulsory certification, this certificate only covers products/services in the approved / certified scope.)

Date of issue: 2020-06-22

Term of validity of this certificate: From 2020-06-22 to 2023-06-21

This certificate remains valid only if the certified organization accepts and passes regular surveillance audits



Scan the QR code to check the validity of this certificate



Representative of The Certification Body



中国认可
国际互认
管理体系
MANAGEMENT SYSTEM
CNAS C169-H

The validity of this certificate could be confirmed via official Website of CNCA (www.cnca.gov.cn) Or the Website of Certification Body (www.cqsg.com) or contact 8611-6218299 ROOM 801, JUCHENGSHANDE BUILDING, NO.212 CENTRAL SHENGENG ROAD, JINAN CITY, SHANDONG PROVINCE, CHINA (250002) SHANDONG GUOJIAN CERTIFICATION CO., LTD.

EMPA Prüfbericht Nr. 5214025580-G

Empa
Lerchenfeldstrasse 5
CH-9014 St. Gallen
T +41 58 765 74 74
F +41 58 765 74 99
www.empa.ch



ILB Helios AG,
Chamerstrasse 175,
CH – 6300 Zug

Prüfbericht Nr. 5214025580-G

Prüfauftrag

Auftraggeber
Probenahme

Analyse von Materialien für Community Masken

ILB Helios AG, Chamerstrasse 175, CH – 6300 Zug
durch Auftraggeber

Prüfobjekt

Kundenreferenz
Ihr Auftrag vom
Eingang des Prüfobjektes
Ausführung der Prüfung
Anzahl Seiten
Beilagen

Aspop Masken, LOT 2020080110

Franz Portmann
27. August 2020
28. August 2020
31. August 2020 bis 18. September 2020
6
Regelung Werbung
AGB Dienstleistungen
Dokument SwissMedic
Empfehlung National COVID-19 Science Task Force
Das restliche Prüfmaterial wird während 2 Jahren archiviert.

Archivierung Material

401 – ell/zep/ioma/bjoy/mha/tiv // Kontroll-Visum: *zep*

Empa, Swiss Federal Laboratories for Materials Science and Technology,
Laboratory for Biomimetic Membranes and Textiles
St. Gallen, 22. September 2020

Prüfleiterin

Leonie El Issawi-Frischknecht

Abteilungsleiter

Prof. Dr. René Rossi

Anmerkung Die Untersuchungsergebnisse haben nur Gültigkeit für das geprüfte Objekt. Bericht und Unterlagen werden 10 Jahre archiviert.

Inhalt

1.	Geprüftes Material (dekl.)	3
1.1	Bilder des Materials	3
2.	Bestimmung der Luftdurchlässigkeit in Anlehnung an ISO 9237 (inkl. Berechnung der Druckdifferenz in Anlehnung an EN 14683:2019-10)	3
2.1	Prüfbedingungen	3
3.	Druck des Spritzwiderstandes in Anlehnung an ISO 22609	4
3.1	Prüfbedingungen	4
4.	Partikelfiltrationseffizienz	4
4.1	Prüfbedingungen	4
5.	Resultate	4
5.1	Anforderungen gemäss Nationalen COVID-19 Science Task Force	5
5.2	Druckdifferenz in Anlehnung an ISO 9237 und in Anlehnung an EN 14683:2019-10	5
5.3	Druck des Spritzwiderstandes in Anlehnung an ISO 22609	5
5.4	Partikelfiltrationseffizienz	6
6.	Ergebnis der durchgeführten Messanalysen	6
7.	Sorgfalt und Haftung:	6
8.	Verwendung des Berichts	6

1. Geprüftes Material (dekl.)

Art Name	Empa Nummer	Farbe	Materialbeschreibung
Aspop Masken, LOT 2020080110	1	blau	Single-Use Medical Face Mask, LOT 2020080110
Erhaltenes Material		50 Masken	

1.1 Bilder des Materials



2. Bestimmung der Luftdurchlässigkeit in Anlehnung an ISO 9237 (inkl. Berechnung der Druckdifferenz in Anlehnung an EN 14683:2019-10)

Mit einem Sauggebläse wird ein definierter Unterdruck erzeugt. Dies führt zu einem Luftfluss durch das aufgelegte und fixierte Material, welche gemessen wird. Basierend auf 10 Messungen wird der Ergebnisbereich bestimmt, welcher die Messunsicherheit der Methode mitberücksichtigt.

2.1 Prüfbedingungen

Art der Messung	Luftdurchflussmessung
Unterdruck	30Pa / 150Pa / 250Pa
Prüffläche	4.9 cm ²
Prüfklima	≥ 4h bei (21 ± 3) °C und (85 ± 5)% rel. Lf.
Anzahl Messungen	10
Lage der Probe	Innenseite gegen Unterdruck
Zustand der Proben	Anlieferungszustand

3. Druck des Spritzwiderstandes in Anlehnung an ISO 22609

Das Prüfobjekt wird auf einem Objekthalter, wie in ISO 22609 beschrieben, aufgebracht. Eine definierte Menge an eingefärbtem synthetischem Speichel (2.01 ± 0.04 g) wird horizontal auf die Aussenseite des Prüfobjekts gesprüht (gesichtsabgewandte Seite). Zusätzlich zur Flüssigkeitsmenge ist die Entfernung zum Aufprall, die Grösse der Blende und die Geschwindigkeit der Flüssigkeit in kontrolliert. Das Prüfobjekt wird bei 12kPa geprüft, was dem Druck beim Husten entspricht. Das Durchdringen von synthetischem Speichel bis auf die Innenseite (Gesichtsseite) des Prüfobjekts wird visuell mit Hilfe eines Kosmetiktuchs festgestellt. Wird das Kosmetiktuch befeuchtet, gilt der Test als "nicht bestanden". Bleibt das Kosmetiktuch trocken, gilt der Test als "bestanden".

3.1 Prüfbedingungen

Prüffläche	4.9 cm ²
Prüfklima	≥ 4h bei (21 ± 3) °C und (85 ± 5)% rel. Lf.
Prüfdruck	12kPa
Prüfflüssigkeit	Synthetischer Speichel rot eingefärbt
Flüssigkeitsmenge	2.01 ± 0.04 g
Anzahl Messungen	10
Lage der Probe	Aussenseite gegen die Spritzdüse
Zustand der Proben	Anlieferungszustand

4. Partikelfiltrationseffizienz

Ein kreisförmiges Muster des Prüfobjekts/textilen Fläche mit Durchmesser von 4.6 cm (Probendurchmesser 6 cm) wird gemessen. Ein neutralisiertes und getrocknetes Aerosol aus Zuckerpartikeln mit einer Größenverteilung über 20 bis 3000 nm Durchmesser und einer Konzentration von $8-9 \cdot 10^5$ dN/dlogD_p/cm³ (normierte Partikelanzahl über die Detektorbandbreite) bei der Partikelgröße höchster Intensität (240 nm) wird über die Probe geleitet. Durch ein Pumpensystem wird ein konstanter Luftdurchfluss von 8 l/min (8 cm/s) durch das Prüfobjekt/die textile Fläche gewährleistet, welcher dem Atemminutenvolumen bei leichter physischer Beanspruchung entspricht und sich an der Norm DIN EN 14683 orientiert. Die durch das Prüfobjekt/die textile Fläche diffundierenden Partikel werden in Echtzeit über ein Partikelmessgerät 'Cambustion DMS500' quantifiziert. Die Partikelfiltrationseffizienz ergibt sich aus den festgestellten Partikelflüssen ohne und mit Prüfobjekt/textile(r) Fläche, nachdem sich ein konstanter Partikelfluss eingestellt hat (nach ca. 2.5 Minuten Exposition) und wird in % über die Bereiche 100 (55-205) nm, 500 (205-750) nm, 1000 (750-1540) nm und 2000 (1540-2740) nm angegeben.

4.1 Prüfbedingungen

Prüffläche	16.6 cm ²
Prüfluftfluss	8 l/min (8 cm/s)
Prüfaerosol	Zuckerlösung (1.5 g/ml) in 24 l/min Luftfluss, neutralisiert
Prüfdauer	ca. 3 min, davon letzte 30 s
Prüfkonzentration	$8-9 \cdot 10^5$ dN/dlogD _p /cm ³ pro Sekunde bei 240 nm Maximum
Anzahl Messungen	5
Lage der Probe	Aussenseite (farbig/glatt/markiert) Richtung Einlass
Zustand der Proben	Anlieferungszustand

5. Resultate

5.1 Anforderungen gemäss Nationalen COVID-19 Science Task Force

Die Maske erfüllt die Anforderungen, wenn folgende Vorgaben erfüllt werden:

Druckdifferenz	≤ 60 [Pa/cm ²]
Druck des Spitzwiderstandes	10 von 10 bestanden bei 12kPa
Partikelfiltrationseffizienz (1 μ m)	$\geq 70\%$

5.2 Druckdifferenz in Anlehnung an ISO 9237 und in Anlehnung an EN 14683:2019-10

Art. Name	Druckdifferenz [Messbereich] [Pa/cm ²]
Aspop Masken, LOT 2020080110	36.3 [34.2; 38.4]

Tabelle 1: Resultate Druckdifferenz. Der Messbereich gibt den Streubereich der Daten an (+/- 1 Standardabweichung festgestellt bei 10 Messungen) Die Anforderung gilt als erfüllt, wenn der Messbereich die geforderte Druckdifferenz mindestens miteinschliesst. Messergebnisse, welche nicht den Anforderungen entsprechen, sind gelb markiert.

5.3 Druck des Spritzwiderstandes in Anlehnung an ISO 22609

Art. Name	Bestandene Muster bei einem Druck des Spritzwiderstandes von 12kPa
Aspop Masken, LOT 2020080110	10 von 10 bestanden

Tabelle 2: Resultate Druck des Spritzwiderstandes. Messergebnisse, welche nicht den Anforderungen entsprechen, sind gelb markiert.

Bild Druck des Spritzwiderstandes



5.4 Partikelfiltrationseffizienz

Art. Name	Ergebnis Partikelfiltrationseffizienz [Ergebnisbereich] in % für			
	100 nm	500 nm	1 µm	2 µm
Aspop Masken, LOT 2020080110	88.6 [86.3; 91.0]	93.6 [92.0; 95.1]	97.7 [97.1; 98.4]	99.8 [99.6; 100]

Tabelle 3: Resultate Partikelfiltrationseffizienz. Der Messbereich gibt den Streubereich der Daten an (+/- 1 Standardabweichung festgestellt bei 5 Messungen) Die Anforderung gilt als erfüllt, wenn der Messbereich die geforderte Filtrationseffizienz mindestens miteinschliesst. Messergebnisse, welche nicht den Anforderungen entsprechen, sind gelb markiert.

6. Ergebnis der durchgeführten Messanalysen

Das geprüfte, ungewaschene Material **entspricht**, in Bezug auf die drei durchgeführten Tests und unter Berücksichtigung der Messunsicherheiten, der Empfehlung der Nationalen COVID-19 Science Task Force. Die Waschbarkeit (Reusability) sowie die Biokompatibilität (Innocuity of the materials) wurden in diesem Prüfauftrag nicht untersucht.

7. Sorgfalt und Haftung:

Die Empa leistet Gewähr für eine sorgfältige, dem aktuellen Stand von Wissenschaft und Technik entsprechende Ausführung der Materialanalysen. Die Messergebnisse beziehen sich nur auf das vom Auftraggeber zur Verfügung gestellte bzw. auf das von der Empa untersuchte Probematerial. Die Empa übernimmt keine Gewähr dafür, dass die Messergebnisse auch für andere Lieferungen des gleichen Materials, Stoffes usw. zutreffen. Die Haftung, gleich aus welchem Rechtsgrund, insbesondere für leichte Fahrlässigkeit, indirekte Schäden und Folgeschäden, wird wegbedungen, soweit dies gesetzlich zulässig ist.

8. Verwendung des Berichts

Die vorliegende Materialanalyse stellt keine Zertifizierung des Produktes des Auftraggebers dar. Der Bericht kann vom Auftraggeber gegenüber Dritten verwendet werden, um darzulegen, dass das Prüfobjekt von der Empa nach den Empfehlungen der Nationalen COVID-19 Science Task Force mit den hierin gemachten Ergebnissen analysiert wurde. Bei der Verwendung des Berichts und insbesondere bei Hinweisen in Werbematerialien ist die "Regelung Werbung mit Empa-Prüfberichten" (vgl. Beilage) einzuhalten. Die Werbebewilligung wird mit diesem Bericht für ein Jahr ab Unterzeichnungsdatum erteilt.

* * * * *